

Moisture meter

Operating Manual humimeter FS2 Grain moisture meter



78,0°F | 6,16%| 456kg/m³| −27,3td| 0,64aw| 51,9%r.H.| 14,8%abs| 100,4g/m²| 09m/s| 4,90Ugl| 1

Your humimeter FS2 at a glance

The main unit



| No. | Name |
|-----|-----------------------------|
| 1 | Auxiliary plate for filling |
| 2 | Measuring chamber |
| 3 | Display |
| 4 | Keypad |
| 5 | Rubber protection cover |



Rear of the main unit



| No. | Name |
|-----|---------------------|
| 1 | Battery compartment |

The display



| No. | Name |
|-----|---|
| 1 | Product type |
| 2 | Moisture content in % ("6.1 How moisture content is defined") |
| 3 | Display symbols |
| 4 | Currently applied offset |
| 5 | Temperature display |

The display symbols

| Symbol | Name |
|---------|---------------------|
| 4 | Enter |
| | Up |
| T | Down |
| 4 | Back |
| 09 | Enter numbers |
| AZ | Enter letters |
| , iller | Continue / go right |
| mage . | Left |
| V | Yes |
| 1/2 | Offset |


| Symbol | Name |
|--------------|------------------------------|
| × | No |
| Û | Change input level |
| OK | ОК |
| P | Change menu |
| Ø. | Enter data |
| <u>"000"</u> | View measurements |
| Æ | Delete measurements |
| Ċ | On/off button, display light |
| | Save measured value |
| | |



The menus

The device has four different menus: product selection, Data Log, offset menu and main menu.

Product selection menu




| No. | Name |
|-----|--------------------------------------|
| 1 | Change menu |
| 2 | Display illumination / device on/off |
| 3 | For changing the product type |

Data Log menu



| No. | Name |
|-----|--------------------------------------|
| 1 | Change menu |
| 2 | Display illumination / device on/off |
| 3 | Save measured value |
| 4 | Show the last recorded values |

Offset menu



| No. | Name |
|-----|--------------------------------------|
| 1 | Change menu |
| 2 | Display illumination / device on/off |
| 3 | Setting the offset |

Main menu

The main menu comprises the following menu items:

- Edit Logs: Manual Logs, Clear Logs
- Options:
 Date/Time, Language, Unlock, °C/°F, BL On Time, Auto Off Time, Materialcalibration, Password, Reset
- Status



Table of contents

| Your | numimeter FS2 at a giance | 2 |
|-----------------------|---|----|
| The ma | ain unit | 2 |
| Rear of the main unit | | |
| The dis | splay | 4 |
| The dis | splay symbols | 4 |
| The me | enus | 5 |
| 1. | Introduction | 10 |
| 1.1 | Information about this operating manual | 10 |
| 1.2 | Limitation of liability | 10 |
| 1.3 | Symbols used in this manual | 11 |
| 1.4 | Customer service | 11 |
| 2. | For your safety | 12 |
| 2.1 | Proper use | 12 |
| 2.2 | Improper use | 12 |
| 2.3 | User qualifications | 12 |
| 2.4 | General safety information | 13 |
| 2.5 | Warranty | 13 |
| 3. | On receipt of your device | 13 |
| 3.1 | Taking the device out of its packaging | 13 |
| 3.2 | Making sure that all of the components have been included | 14 |
| 3.3 | Inserting batteries | 14 |
| 4 . | Using the device - Basics | 15 |
| 4.1 | Switching the device on | 15 |
| 4.2 | Automatic calibration | 15 |
| 4.3 | Selecting the product type | 16 |
| 4.4 | Taking a measurement | 16 |
| 4.5 | Switching the device off | 16 |

| 5. | The measuring process | 17 |
|--------|---|----|
| 5.1 | Preparing a measurement | 17 |
| 5.2 | Taking a measurement | 18 |
| 5.3 | Saving individual readings | 19 |
| 5.4 | Saving several readings (a measurement series) at the same time | 20 |
| 5.5 | Viewing individual readings | 22 |
| 5.6 | Viewing individual readings from a series of measurements | 22 |
| 5.7 | Deleting all measured values (data log) | 23 |
| 5.8 | Deleting individual measurement series | 23 |
| 5.9 | Deleting individual values from a single series of measurements | 24 |
| 5.10 | Offset function | 25 |
| 5.10.1 | Setting the offset | 25 |
| 6. | Product types | 27 |
| 6.1 | How moisture content is defined | 28 |
| 7. | Checking the device's status | 29 |
| 8. | Configuring the device | 30 |
| 8.1 | Adjust the date/time | 30 |
| 8.2 | Selecting a language | 31 |
| 8.3 | Activating options | 31 |
| 8.4 | Deactivating options | 32 |
| 8.5 | Selecting °C/°F | 32 |
| 8.6 | Reducing the device's power consumption | 33 |
| 8.6.1 | Configuring the display illumination time | 33 |
| 8.6.2 | Configuring automatic switch-off | 33 |
| 8.7 | Configuring the material calibration function | 34 |
| 8.8 | Changing the password | 34 |
| 8.9 | Resetting the device to its factory settings | 35 |
| | , , | |



| 9.1 | Changing batteries | 35 |
|------|------------------------------|----|
| 9.2 | Checking the calibration | 36 |
| 9.3 | Care instructions | 36 |
| 9.4 | Cleaning the device | 36 |
| 10. | Faults | 37 |
| 11. | Storage and disposal | 38 |
| 11.1 | Storing the device | 38 |
| 11.2 | Disposing of the device | 38 |
| 12. | Device information | 39 |
| 12.1 | EC declaration of conformity | 39 |
| 12.2 | Technical data | 43 |

1. Introduction

1.1 Information about this operating manual

This operating manual is designed to enable you to use the humimeter FS2 safely and effectively. It is part of the device, has to be stored nearby and must be easily accessible to users at all times.

All users are required to carefully read and make sure that they have understood this operating manual before using the humimeter FS2. All of the safety and operating instructions detailed in this manual have to be observed to ensure the safety of the device.

1.2 Limitation of liability

All of the information and instructions provided in this operating manual have been compiled on the basis of the current standards and regulations, the state of the art, and the extensive expertise and experience of Schaller Messtechnik GmbH.

Schaller Messtechnik GmbH does not accept any liability for damage associated with the following, which also voids the warranty:

- Non-observance of this operating manual
- Improper use
- Inadequately qualified users
- · Unauthorised modifications
- Technical changes
- Use of unapproved spare parts

This fast measuring procedure can be affected by a range of different factors. For this reason, we recommend periodically checking the device's measurements with a standardised oven-drying method.

We, as the manufacturer, do not accept any liability for any incorrect measurements and associated consequential damage.



1.3 Symbols used in this manual

All of the safety information provided in this manual is shown with a corresponding symbol.



ATTENTION

It is essential to observe this warning. Non-compliance can lead to damage to property or equipment.



Information

This symbol indicates important information that enables users to use the device more efficiently and cost effectively.

1.4 Customer service

For technical advice, please contact our customer service department at

Schaller Messtechnik GmbH Max-Schaller-Straße 99 A - 8181 St.Ruprecht an der Raab

Telephone: +43 (0)3178 28899 Fax: +43 (0)3178 28899 - 901

E-mail: info@humimeter.com Internet: www.humimeter.com

© Schaller Messtechnik GmbH 2023



2. For your safety

The device complies with the following European directives:

- Restriction of Hazardous Substances in Electrical and Electronic Equipment (RoHS)
- Electromagnetic compatibility (EMC)

The device corresponds to state-of-the-art technology. However, it is still associated with a number of residual hazards.

These hazards can be avoided through strict observance of our safety information.

2.1 Proper use

- Easy to use device for quickly measuring the moisture content of cereals
- The device must only be used for taking measurements on the products defined in the following sections of this manual (see "The displayed measurement value now deviates from the standard calibration!").

2.2 Improper use

- The device is not suitable for measuring mouldy material.
- The device is not waterproof and must be protected from water and fine dust.

2.3 User qualifications

The device must only be operated by people who can be expected to reliably take the measurements. The device must not be operated by people whose reaction times may be slowed due to, e.g. the use of drugs, alcohol or medication.

All persons using this device must have read, understood and follow the instructions provided in the operating manual.



2.4 General safety information

The following safety information has to be observed at all times to avoid damage to objects and injury to people:

- Remove the batteries if the device isn't used for a prolonged period of time (4 weeks).
- In case of damages or loose parts on the device, remove the batteries and contact Schaller Messtechnik GmbH or your dealer.

All of the device's technical features have been inspected and tested before delivery. Every device has a serial number. Do not remove the tag with the serial number.

2.5 Warranty

The warranty does not apply to:

- Damage resulting from non-observance of the operating manual
- · Damage resulting from third-party interventions
- Products that have been used improperly or modified without authorisation
- Products with missing or damaged warranty seals
- Damage resulting from force majeure, natural disasters, etc.
- Damage from improper cleaning
- Batteries older than six months.

3. On receipt of your device

3.1 Taking the device out of its packaging

- Take the device out of its packaging.
- Next, make sure that it is not damaged and that no parts are missing.

3.2 Making sure that all of the components have been included

Make sure that all of the components have been included by checking the package contents against the following list:


- humimeter FS2
- 4 pieces of AA Alkaline batteries
- Digital scale 500 grams
- Measuring cup 0.5 liter
- Plastic case
- Rubber protection cover
- · Operating manual

3.3 Inserting batteries

- 1. Remove the rubber protection cover. To do so, hold the rubber protection cover at the upper side and pull it over. If your device is provided with an optional USB port, remove the protection cap of the USB socket before (figure 1 and 2).
- imetr



2. Take hold of the device with one hand, press your thumb onto the engraved area of the battery compartment (1) and drag downwards (2) (figure 3).



- » As soon as all batteries have been inserted, the device switches on automatically.
- 4. Push the battery cover onto the housing until it clicks into place. Then mount the rubber protection cover onto the housing, beginning at the end where the battery compartment is situated (figure 5).









4. Using the device - Basics


4.1 Switching the device on

- Press the button for 3 seconds.
- The display will then show the status indicator (figure 6).
- » After inserting the batteries, the device switches on automatically.



4.2 Automatic calibration

- » The display will show the message Adjust? (figure 7).
- Make sure that the measuring chamber of the device is empty and place the device on a level table.
- 2. Confirm by pressing .
 - » The display will now appear as shown in figure 8.
 - » The bar will run upwards. During this period, the device must remain on the table without external influence.
 - » which only takes a couple of seconds to complete.
 - » Once completed, the device will show the measuring window (see "Product selection menu" page 5).





4.3 Selecting the product type

To do so: The device has to be in the product selection menu (figure 9).

For an overview of the different product types and the criteria for selecting them, please refer to "The displayed measurement value now deviates from the standard calibration!".

- 1. Press the ♥ or ♠ button to move from one product type to the next Or
- 2. Press the or button for 3 seconds to open the product type overview (figure 10).
- Use the arrow keys to move from one product type to the next
- and keep any of them pressed to scroll through the types.
- 5. Confirm your selection by pressing
 - » The product type you selected will now be shown at the top of the display.

4.4 Taking a measurement

 For information on how to take a measurement, see section "5. The measuring process".

4.5 Switching the device off

To do so: The device has to be in the product selection or Data Log menu. It is not possible to switch off the device when it is in the main menu.

• Press the 🖒 button for 3 seconds.





5. The measuring process

5.1 Preparing a measurement

To do so: The device has to have nearly the same temperature than the product being measured. It is recommended to let your humimeter device adjust to the surrounding temperature of the material being measured for at least 30 minutes.

- Place the empty and clean measuring cup (0.5 liter) on the switched-off scale (figure 11). Then switch on the scale.
- » The balance must display 0.0 g with the empty measuring cup on it. The measuring cup must not be weighed.
- Check whether the measuring chamber of the device is empty. When the device is switched on, there must not be any material in it.
 - Empty the instrument and clean the measuring chamber if necessary (see "9.4 Cleaning the device").
- 3. Switch on the device (see "4.1 Switching the device on").
- 4. Perform the automatic calibration (see "4.2 Automatic calibration").
- 5. Select the required product type (see "The displayed measurement value now deviates from the standard calibration!") by pressing the or button (see "4.3 Selecting the product type").







5.2 Taking a measurement

To do so: The device has to have nearly the same temperature than the product being measured.

- Fill the measuring cup with the filling quantity displayed in the product type name (+/- 1.0 g) (figure 15) (see "The displayed measurement value now deviates from the standard calibration!")
- 2. Now slowly and evenly fill the measuring chamber of the device with the material being measured (figure 15).
 - » For the filling, no funnel or similar device may be used.
- 3. The device will now display the moisture content (figure 16).
 - » The displayed value flashes when the moisture content exceeds the measuring range of the selected product type (figure 17). A flashing value signals a decreasing accuracy of the measurement. The measuring range is dependent on the product type (see "The displayed measurement value now deviates from the standard calibration!").
 - Once the reading has been taken, it can be saved on the device (see "5.3 Saving individual readings" or "5.4 Saving several readings (a measurement series) at the same time").
 - » It is possible to apply an offset to the displayed measurement value (see "5.10 Offset function").
- 4. Empty the device and make sure that there are no residues in the measuring chamber.
 - » Clean the measuring chamber if necessary (see "9.4 Cleaning the device").









i.

Information - Measuring accuracy

This rapid and non-destructive measuring procedure allows you to quickly take several moisture readings of the same sample material. When saving the individual readings, the device will automatically calculate the readings' average (see "5.4 Saving several readings (a measurement series) at the same time").





Always make sure to select the correct product type and the correct filling quantity for the material you are measuring. This prevents taking incorrect readings (see "10. Faults").

5.3 Saving individual readings

The device is configured in such a way that the device will save a reading every time a button is pressed.

To do so: The device has to be in the Data Log menu (see "Data Log menu" page 5).

- 1. Press .
 - » The display will now appear as in figure 19 and the disc symbol will be preceded by the digit one.
- 2. Press to enter a name for the saved reading and to finish the measuring process.
 - » The display will now appear as shown in figure 20.
- 3. The data you have inputted can be overwritten at any time.
- 4. Inputting letters:

Press and hold A ... to quickly scroll to the required letter and either press it for 3 seconds or pres to confirm the selected letter (figure 21).

5. Inputting numbers:

Press and hold **1 ... 9** to quickly scroll to the required number and either press it for 3 seconds or press **4** to confirm the selected number.

6. Moving forward/back:

Press to switch to another input level. Press to move forward or back.

- 7. Confirm your entry by pressing 🚚.
 - » The data you entered has been saved.









5.4 Saving several readings (a measurement series) at the same time

To do so: The device has to be in the Data Log menu (see "Data Log menu" page 5).

- Take several measurements of the same sample material (see "5. The measuring process").
- 2. To save a reading, press as soon as the reading has been taken.
 - » The display will now appear as shown in figure 22. This number shows the number of readings that have already been saved.
- 3. Press to enter a name for the saved series of measurements and to finish the measuring process.
 - » The display will now appear as shown in figure 23.
- 4. The data you have inputted can be overwritten at any time.
- 5. Inputting letters:

Press and hold A ... to quickly scroll to the required letter and either press it for 3 seconds or press to confirm the selected letter (figure 24).







- 6. Inputting numbers:
 - Press and hold **1 1 1 9** to quickly scroll to the required number and either press it for 3 seconds or press **4** to confirm the selected number.
- 7. Moving forward/back:

Press to switch to another input level. Press to move forward or back

- 8. Confirm your entry by pressing 🚚.
 - The data you entered has been saved.
 - » The device automatically determines the average moisture content of the saved measuring values.



» The display will show the following information:




| No. | Name |
|-----|---|
| 1 | Name of the measurement series (editable) |
| 2 | Temperature (average) |
| 3 | Date & start time of the measurement series |
| 4 | Date & end time fo the measurement series |
| 5 | Number of saved readings |
| 6 | Product type |
| 7 | Device name |
| 8 | Moisture content (average) |

5.5 Viewing individual readings

To do so: You must have saved a reading (e.g. 1 log) The display will now appear as shown in figure 25.

- 1. Press '000'.
- - » The display will now appear as shown in figure 26.
 - » Press 👫 to leave this screen.





5.6 Viewing individual readings from a series of measurements

To do so: You must have saved a series of measurements (e.g. 2 logs).

The display will now appear as shown in figure 27.

- 1. Press '000'.
- 2. Select the required reading. To do so, press or
 - » The display will now appear as shown in figure 28.
- 3. Press to switch to another input level.
 - » The display will now appear as shown in figure 29.
- 4. Press 'm' again.
 - » The display will now appear as shown in figure 30.
- 5. Navigate to the required reading (No.: 1, No.: 2, No.: 3). To do so, press or or or.
- 6. Press 👫 to leave this screen.














5.7 Deleting all measured values (data log)

To do so: You must have taken and saved one or several readings.

- 1. Press **\$\infty\$** twice or hold for 2 seconds.
- 2. Select **Edit Logs** (figure 31). To do so, press or and confirm by pressing .
- 3. Select Clear Logs (figure 32). To do so, press T or and confirm by pressing .
 - » The display will show the message clear? (figure 33).
- 4. Confirm by pressing 📢.
 - » The data log has been deleted.
- 5. Press **1** to leave the **Edit Logs** menu.
- 6. Press to leave the main menu.








5.8 Deleting individual measurement series

To do so: You must have saved a measured value (e.g. 1 log) or a series of measurements (e.g. 3 logs). The display will now appear as shown in figure 34.

- 1. Press '0-0'.
 - » The display will now appear as shown in figure 35.
- 2. Select the required reading. To do so, press **T** or
- 3. Press **\$\iiig\$** to switch to another input level.
 - » The display will now appear as shown in figure 36.
- 4. Press 🧵.







- » The display will then show the message clear? (figure 37).
- 5. Confirm by pressing **...**.
 - » The value has been deleted.



5.9 Deleting individual values from a single series of measurements

To do so: You must have saved a series of measurements comprising at least 2 logs. The display will now appear as shown in figure 40.

- 1. Press '000'.
 - » The display will now appear as shown in figure 39.
- 2. Select the required reading. To do so, press T or
- 3. Press to switch to another input level.
 - » The display will now appear as shown in figure 40.
- 4. Press '000'.
 - » The display will now appear as shown in figure 41.
- 6. Press to switch to another input level.
 - » The display will now appear as shown in figure 42.
- 7. Press I to delete the value shown.
 - » The display will then show the message clear? (figure 43).
- - » The value has been deleted.
















5.10 Offset function

By changing the offset, the displayed measurement values can be adapted to other norms/standards. The displayed measuring value is corrected by the entered offset.

Example:

An offset of 1.5 % applied to a measurement value of 10.0 % results in a displayed measurement value of 11.5 %.

An offset of - 0.5 % applied to a measurement value of 10.0 % results in a displayed measurement value of 9.5 %.

5.10.1 Setting the offset

To do so: The device has to be switched on and be in the product selection menu.

- 1. Select the required product type (see "6. Product types") by pressing the or button (see "4.3 Selecting the product type").
- 2. Press 🛊 twice to change to the offset menu.
- 3. Press 🔀 .
 - » The display will now show the material calibration menu for the selected product type (figure 45).
 - » The offset is part of the material calibration menu.



OA

300g Wheat

- 4. Select **Offset**. To do so, press \P or $\underline{\mathbb{A}}$ and confirm by pressing \blacksquare
- 5. The data you have inputted can be overwritten at any time.
- 6. Inputting numbers:

Press and hold not to the required number and either press it for 3 seconds or press to confirm the selected number (figure 46).




- Setting a negative offset is also possible!
 To do so, insert a minus sign before the first digit.
- » Take care of the position of the comma to prevent setting an offset that is too high!
- 7. Moving forward:
 To move forward, press

8. Moving back:

Press to switch to another input level. To move back, press

- - » The offset has been saved.
- 10. Press 4 to leave the material calibration menu.










6. Product types

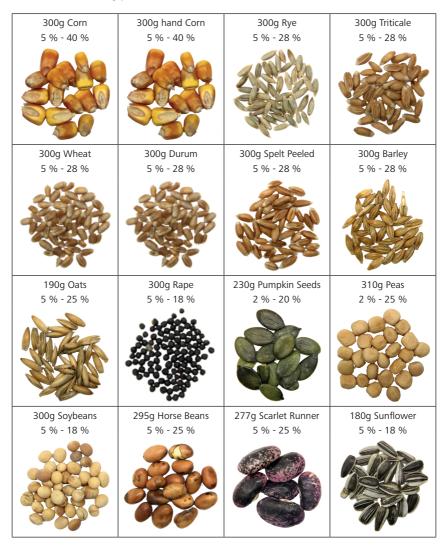

| 300g Rice peeled | 250g Rice unpeeled | 300g Rice brown | 300g Buckwheat |
|--|--|---------------------|--|
| 5 % - 25 % | 4 % - 30 % | 4 % - 26 % | peeled |
| | | | 5 % - 18 % |
| A CONTRACTOR OF THE PARTY OF TH | Pallers. | | Color Service |
| | A STATE OF THE STA | 000000 | O STATE OF THE STA |
| | | W 2000 | |
| | | | |
| and make | | 33.0 | 82000 g |
| 300g Buckwheat | 300g Millet | 300g Sorghum Millet | 200g Jatropha |
| unpeeled | 5 % - 15 % | 5 % - 25 % | 5 % - 18 % |
| 3 % - 25 % | | | |
| | ande. | - 040 | 4 |
| 90779 | 430 | 200 | |
| 2023 | 800000000000000000000000000000000000000 | 2000 | |
| | | | |
| | 2 6 6 6 6 6 6 6 6 6 6 6 6 6 6 6 6 6 6 6 | | |
| | 3,540 | 2000 | |
| Referenz | _ | | |
| Keterenz | | | |
| ! Only for testing the | | | |
| moisture meter! | | | |
| | | | <u> </u> |

On request, Schaller Messtechnik GmbH can develop customer-specific characteristic curves for special product types. It is also possible to subsequently enter optionally available characteristic curves into the device.

6.1 How moisture content is defined

The device measures and shows a material's moisture content. The moisture content readings it displays are calculated in relation to the material's overall mass:

$$\%WG = \frac{M_n - M_t}{M_n} \times 100$$

M_n: Mass of the sample with average moisture content

M_.: Mass of the sample with zero moisture content

%WG: Moisture content (in accordance with the corresponding product norms)



7. Checking the device's status

- 1. Press Twice or hold for 2 seconds.
- 2. Select **Status**. To do so, press \P or $\stackrel{\bot}{\blacksquare}$ and confirm by pressing $\stackrel{\longleftarrow}{\blacksquare}$.
 - » The display will then show the status indicator humimeter.
 - » The display will show the following information:



| No. | Name |
|-----|------------------|
| 1 | Serial number |
| 2 | Software version |
| 3 | Battery status |
| 4 | Memory status |

- 3. Confirm by presssing **...**.
- 4. Press 😱 to leave the main menu.

8. Configuring the device

8.1 Adjust the date/time

- 1. Press 🔓 twice or hold for 2 seconds.
- 2. Select **Options**. To do so, press \P or $\stackrel{\blacktriangle}{\blacksquare}$ and confirm by pressing $\stackrel{\blacksquare}{\blacksquare}$.
- 3. Select **Date/Time**. To do so, press **T** or **A** and confirm by pressing **4**.
 - » The display will now appear as shown in figure 48.
 - » The format for the date is **DD-MM-YY** (Day-Month-Year).
- » The format for the time is hh:mm:ss (Hour:Minutes:Seconds).

4. Inputting numbers:


5. Moving forward:

To move forward between **DD-MM-YY** and **hh:mm:ss**, press **b**.

6. Moving back:

Press to switch to another input level. To move backward between **DD-MM-YY** and **hh:mm:ss**, press ...

- 7. Confirm the date/time by pressing **I**K.
 - » The settings have been saved.
- 8. Press 4 to leave the **Options** menu.
- 9. Press to leave the main menu.





8.2 Selecting a language

- 1. Press \$\infty\$ twice or hold for 2 seconds.
- 2. Select **Options**. To do so, press \P or $\begin{tabular}{l} \bot \\ \end{tabular}$ and confirm by pressing $\begin{tabular}{l} \longleftarrow \\ \end{tabular}$.
- 4. Navigate to the required language. To do so, press **T** or **A** and confirm by pressing **A**.
 - » The settings have been saved.
- 5. Press 4 to leave the **Options** menu.
- 6. Press to leave the main menu.

8.3 Activating options

To do so: Some of the options must be deactivated.

- 1. Press twice or hold for 2 seconds.
- 2. Select **Options**. To do so, press \P or \red and confirm by pressing \red .
- 3. Select **Unlock**. To do so, press \P or \dbelowdisplay and confirm by pressing \ddelowdisplay .
 - » The display will now appear as shown in figure 50.
 - » On delivery, the four-digit password is the device's serial number.
- 4. Inputting numbers:

Press and hold to quickly scroll to the required number and either press it for 3 seconds or press to confirm the selected number (figure 51).



Press to switch to another input level. To move back, press

- 6. Confirm the four-digit password by pressing **[] K**.
 - » The setting has been saved.





- » The °C/°F, BL On Time, Auto Off Time, Materialcalibration, Password, Reset options are now activated.
- 7. Press 4 to leave the **Options** menu.
- 8. Press **\$\Pi\$** to leave the main menu.

8.4 Deactivating options

Once the device has been switched restarted, the °C/°F, BL On Time, Auto Off Time, Materialcalibration, Password, Reset options will be deactivated again.

8.5 Selecting °C/°F

To do so: All of the options must be activated (see "8.3 Activating options").

- 1. Press **twice** or hold for 2 seconds.
- 2. Select **Options**. To do so, press \P or $\begin{cal} \blacksquare \end{cal}$ and confirm by pressing $\begin{cal} \blacksquare \end{cal}$.
- 3. Select °C/°F. To do so, press \P or $black ext{and confirm by pressing } black black ext{.}$
- 4. Navigate to the required temperature scale, i.e. Celsius (°C) or Fahrenheit (°F). To do so, press or in and confirm by pressing in the confirmation in the confirma
 - » The setting has been saved.
- 5. Press | to leave the **Options** menu.
- 6. Press **t** to leave the main menu.



8.6 Reducing the device's power consumption

8.6.1 Configuring the display illumination time

To do so: All of the options must be activated (see "8.3 Activating options").

- 1. Press \$\infty\$ twice or hold for 2 seconds.
- 2. Select **Options**. To do so, press \P or $dag{1}{4}$ and confirm by pressing $dag{4}$.
- 3. Select **BL On Time**. To do so, press **T** or **a** and confirm by pressing **4**.
- 4. Select the required display illumination period (30 seconds, 2 minutes, 5 minutes, 10 minutes). To do so, press or in and confirm by pressing.
 - » The setting has been saved.
- 5. Press 4 to leave the **Options** menu.
- 6. Press **t** to leave the main menu.

8.6.2 Configuring automatic switch-off

To do so: All of the options must be activated (see "8.3 Activating options").

- 1. Press **\$\infty\$** twice or hold for 2 seconds.
- 2. Select **Options**. To do so, press \P or \red and confirm by pressing \red .
- 3. Select Auto Off Time. To do so, press \P or line and confirm by pressing line.
- 4. Select the period of time you want the device to stay switched on (3 minutes, 5minutes, 10 minutes). To do so, press \$\textbf{T}\$ or \$\textbf{\Lambda}\$ and confirm by pressing \$\textbf{\Lambda}\$.
 - » The setting has been saved.
- 5. Press 4 to leave the **Options** menu.
- 6. Press to leave the main menu.

8.7 Configuring the material calibration function

The type calibration function is described in a separate operating manual.

8.8 Changing the password

To do so: All of the options must be activated (see "8.3 Activating options").

- 1. Press twice or hold for 2 seconds.
- 2. Select **Options**. To do so, press \P or $dag{1}{4}$ and confirm by pressing $dag{4}$.
- 3. Select **Password**. To do so, press \P or $\begin{subarray}{c} \bot \end{subarray}$ and confirm by pressing $\begin{subarray}{c} \bot \end{subarray}$.
 - » The display will show the current password.
- 4. Overwrite the current password. To do so, press and hold \(\bigcap_{\text{...9}} \) to quickly scroll to the required number and either press it for 3 seconds or press \(\bigcap_{\text{...1}} \) to confirm the selected number.

Moving back:

Press to switch to another input level.

- 5. Confirm the new four-digit password by pressing **IK**.
 - » The setting has been saved.
- 6. Press | to leave the **Options** menu.
- 7. Press **t**o leave the main menu.



8.9 Resetting the device to its factory settings

To do so: All of the options must be activated (see "8.3 Activating options").

- 1. Press **\$\infty\$** twice or hold for 2 seconds.
- 2. Select **Options**. To do so, press \P or $dag{1}{4}$ and confirm by pressing $dag{4}$.
- 3. Select **Reset**. To do so, press **T** or **A** and confirm by pressing **4**.
 - » The display will then show the message Reset? (figure 52).
- 4. Confirm by pressing **.
 - » The device will now be reset to its factory settings. All of your personal settings will be lost.
 - » The display will show the status indicator humimeter (figure 53).
 - » Resetting the device will not affect the saved measuring values.





9. Cleaning and maintenance

Regularly cleaning and maintaining the device will ensure that it will have a long service life and stay in good condition.

9.1 Changing batteries

The device constantly monitors the charge level of the batteries. The current battery status is shown on the status screen.

If the battery's charge is very low, the battery symbol will be shown with an exclamation mark. In that case, the batteries must be changed immediately (figure 55).

For changing the batteries, see section "3.3 Inserting batteries".

As the device's user, you are responsible by law for properly disposing of all used batteries, which must not be disposed of as domestic waste (Battery Directive).





9.2 Checking the calibration

The calibration check is described in a separate test equipment operating manual.

9.3 Care instructions

- Do not leave the device out in the rain. The device is not waterproof.
- Do not expose the device to extreme temperatures.
- Protect the device from strong mechanical shocks and loads.
- · Remove the batteries after the harvesting season.

9.4 Cleaning the device



ATTENTION

Do not clean with fluids

Water or cleaning fluid getting inside the device can destroy the device.

Only clean with dry materials.

Plastic housing

• Clean the plastic housing with a dry cloth.

Measuring chamber

Clean the measuring chamber with a soft brush.



10. Faults

If the measures listed below fail to remedy any faults or if the device has faults not listed here, please contact Schaller Messtechnik GmbH.

| Fault | Cause | Remedy |
|-----------------|--|---|
| Measuring error | The temperature of the material being measured is too low or high. I.e. the material's temperature is lower than 0 °C or higher than +40 °C. | The temperature of the material being measured has to be between 0 °C and +40 °C. |
| | Temperature discrepancy between device and material being measured | Let the temperature adjust to the material being meas- ured (permitted difference of max. 3 °C). |
| | Wrong product type | Check whether you have selected the right product type (product) before taking a reading (see "The displayed measurement value now deviates from the standard calibration!"). |
| | Wrong filling quantity | Exactly fill in the filling quantity displayed in the product type name (+/- 1.0 gram). |
| | Mouldy or rain wet material | The accuracy decreases significantly. |
| | Stored and fermented corn from whole grain silage | May lead to a too high displayed measuring value. |
| | Frozen material or material mixed with snow | The accuracy decreases significantly. |
| | Contaminated material | Highly contaminated material such as long ears of barley or foreign material can strongly influence the measuring result. |

| Fault | Cause | Remedy |
|-------|----------------|---|
| | Entered offset | An entered offset leads to deviations on the displayed measured value. If the deviation does not match your reference procedure, enter an offset corresponding to the difference or set the offset to 0.0 (see "5.10 Offset function") to restore the factory characteristic curve. |

11. Storage and disposal

11.1 Storing the device

The device must be stored as follows:

- Do not store outdoors.
- Store in a dry and dust-free place.
- Protect the device from sunlight.
- Avoid mechanical shocks/loads.
- Remove the batteries if the device isn't used for a period of 4 weeks or longer
- Storage temperature: -20 °C to +60 °C

11.2 Disposing of the device



Devices marked with this symbol are subject to Directive 2012/19/EU of the European Parliament and of the Council of 4 July 2012 on waste electrical and electronic equipment (WEEE).

If the device is being operated outside the European Union, the national regulations on the disposal of such devices that apply in the country of use must be observed.

Electronic devices must not be disposed of as domestic waste.

The device must be disposed of appropriately using appropriate collection systems.



12. Device information

12.1 EC declaration of conformity



Name/ Adresse des Herstellers: Schaller Messtechnik GmbH Name/ address of manufacturer: Max-Schaller-Straße 99

A - 8181 St. Ruprecht

Produktbezeichnung: humimeter

Product designation:

Typenbezeichnung: FS1; FS1.1; FS2; FS3; FS4; FS4.1; FS4.2; BP1

Type designation:

Produktbeschreibung: Messgerät zur Bestimmung des Wassergehalts in Lebens-

mitteln

Product description Measuring instrument for determining the water content in

foodstuffs

Das bezeichnete Produkt erfüllt die Bestimmungen der Richtlinien:

The designated product is in conformity with the European directives:

EMV - Richtlinie 2014/30/EC EMC Directive 2014/30/EU RoHS - Richtlinie 2011/65/EG RoHS-Directive 2011/65/EU

Die Übereinstimmung des bezeichneten Produktes mit den Bestimmungen der Richtlinien wird durch die vollständige Einhaltung folgender Normen nachgewiesen:

Full compliance with the standards listed below proves the conformity of the designated product with the provisions of the above-mentioned EC Directives:

EN 61326-1:2013 Elektrische Mess-, Steuer-, Regel- und Laborgeräte - EMV-An-

forderungen

Electrical equipment for measurement, control, and laboratory

use - EMC requirements

EN IEC 63000:2019-05 ersetzt / replaced EN 50581:2012

Technische Dokumentation zur Beurteilung von Elektro- und Elektronikgeräten hinsichtlich der Beschränkung gefährliche Stoffe

Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous

substances

Für das angeführte Produkt ist eine vollständige Dokumentation mit Betriebsanleitung in Originalfassung

For the mentioned product a complete documentation with manual of instruction in original version is available.

Bei Änderungen, die nicht vom Hersteller spezifiziert sind, verliert diese Konformitätserklärung die Gültigkeit.

In case of any changes not agreed upon with the manufacturer, this declaration of conformity loses its validity.

St. Ruprecht a.d. Raab, 31.07.2022

Bernhard Maunz

Rechtsverbindliche Unterschrift des Ausstellers Legal binding signature of the issuer





DECLARATION OF CONFORMITY

Name/ address of manufacturer: Schaller Messtechnik GmbH

Max-Schaller-Straße 99 A – 8181 St. Ruprecht

Product designation: humimeter

Type designation: FS1; FS1.1; FS2; FS3; FS4; FS4.1; FS4.2; BP1

Product description: Measuring instrument for determining the water content in

foodstuffs

The designated product is in conformity with the following directives:

• Electromagnetic Compatibility Regulations 2016 Great Britain

 RoHS-Directive 2011/65/EU Directive on the restriction of the use of certain hazardous substances in electrical and electronic equipment

Full compliance with the standards listed below proves the conformity of the designated product with the provisions of the above-mentioned Directives:

EN 61326–1:2013 Electrical equipment for measurement, control, and laboratory

use - EMC requirements

EN IEC 63000:2019-05

replaced EN 50581:2012 Technical documentation for the assessment of electrical and electronic products with respect to the restriction of

hazardous substances.

For the mentioned product, a complete documentation with manual of instruction in original version is available.

In case of any changes not agreed upon with the manufacturer, this declaration of conformity loses its validity.

St. Ruprecht a.d. Raab, 31.07.2022

Mesketcht / uminfeter om
Schaller Negate 1 (Grubb
An - 5 major | Grubb |
An - 8 major | Grubb |
An - 8 major | Grubb |
Bernhard Maunz
Legal binding signature of the issuer



12.2 Technical data

| Display resolution | 0.1 % moisture content, 0.5 °C/°F temperature |
|--------------------------|--|
| Measuring range | 5 % to 40 % moisture content (depending on product type) |
| Operating temperature | 0 °C to +40 °C |
| Storage temperature | -20 °C to +60 °C |
| Temperature compensation | Automatic |
| Data memory | Up to 10,000 measuring values |
| Power supply | 4 x 1.5 Volt AA Alkaline batteries |
| Current consumption | 60 mA (incl. display illumination) |
| Menu languages | English, German, French, Italian, Spanish, Portuguese, Czech, Polish, Russian, International |
| Display | 128 x 64 illuminated matrix display |
| Device dimensions | 260 x 70 x 250 mm |
| Device weight | 1,300 g |
| Case dimensions | 450 x 360 x 106 mm |
| Weight of device + case | 3,180 g |
| Device IP rating | IP 40 |



Schaller Messtechnik develops, produces and sells professional moisture meters and turnkey solutions.

Schaller Messtechnik GmbH

Max-Schaller-Straße 99, A - 8181 St. Ruprecht an der Raab Tel +43 (0)3178 - 28899, Fax +43 (0)3178 - 28899 - 901 info@humimeter.com, www.humimeter.com